



Human Orosomucoid ELISA Quantitation Kit

Manual

Catalog number: PRO-22927F

For the quantitative determination of human Orosomucoid levels in serum or other biological samples.

This kit is for research use only, and is not for use in diagnostic procedures.

PROALT - Protein Alternatives SL

C/ Santiago Grisolia, 2
PTM – Parque Científico de Madrid
28760 Tres Cantos, Madrid. SPAIN
Phone / Fax: +34 91 804 79 74
Email: info@proteinalternatives.com
<http://www.proteinalternatives.com>

Kit Contents:

Coating Antibody (Catalog # 15-288-22927F)

Affinity-purified Chicken anti-Human Orosomuroid
Concentration: 0.5 mg/ml
Volume: 1 ml
Working Dilution: 1/100

Calibrator (Catalog # 10-288-22927F)

Pure Human Orosomuroid Antigen
Concentration: 5 mg/ml
Quantity: 100 ug
Working Range: 250-3.9 ng/ml

HRP Detection Antibody (Catalog # 27-288-22927F)

Affinity-purified Chicken anti-Human Orosomuroid – HRP Conjugate
Concentration: 0.571 mg/ml
Quantity: 100 ug

Buffers, Substrate and Plates not included.

Notes:

Range of Detection: 250-3.9 ng/ml

Storage: Aliquot to 10 tubes stored at -20° C. Shelf life is one year from date of receipt.

Assay Condition: The kit performance has been optimized for the stated protocol using the materials listed and standard dilutions from 250-3.9 ng/ml of human Orosomuroid. *For alternative assay conditions, the operator must determine appropriate dilutions of reagents.* ELISA assay reactivity is sensitive to any variation in operator, pipetting and washing techniques, incubation time or temperature, composition or reagents, and kit age. Adjustments may be required to position the standard curve and/or samples in the desired detection range.

Specificity: By immunoelectrophoresis and ELISA the antibodies in this kit react specifically with human Orosomuroid, not with other human serum proteins. The following factors prepared in the detection range of this kit, 250-3.9 ng/mL were assayed and exhibited no cross-reactivity or interference.

Human Serum Albumin
Human Transferrin
Human IgG

Country of Origin: United States of America

Assay Use: For in vitro laboratory use only. Not for any clinical, therapeutic, or diagnostic use in humans or animals. Not for animal or human consumption.

Human Orosomuroid Quantitative ELISA Protocol

Buffer Preparation

1. Prepare the following buffers:
 - A. Coating Buffer, 0.05 M Carbonate-Bicarbonate, pH 9.6
 - B. Wash Solution, 50 mM Tris, 0.14 M NaCl, 0.05% Tween 20, pH 8.0
 - C. Blocking (Postcoat) Solution, 1% Milk in PBS
 - D. Sample/Conjugate Diluents, 1% Milk in PBS
 - E. Enzyme Substrate, TMB (OPD or ABTS can be used)
 - F. Stopping Solution, 2 M H₂SO₄ or other appropriate solution

Step-by-Step Method (Perform all steps at room temperature)

1. Coat with Capture Antibody
 - A. Determine the number of single wells needed. Standards, samples, blanks and/or controls should be analyzed in duplicate. Insert the required number of microtiter wells trips into a holder.
 - B. Dilute 1 mcl capture antibody to 100 mcl Coating Buffer for each well to be coated. (Example: for 32 wells dilute 34 mcl to 3.4 ml)
 - C. Incubate coated plate for 60 minutes
 - D. After incubation, aspirate the Capture Antibody solution from each well.
 - D. Wash each well with Wash Solution as follows:
 1. Fill each well with Wash Solution
 2. Remove Wash Solution by aspiration
 3. Repeat for a total of 3 washes.
2. Blocking (Postcoat)
 - A. Add 200 mcl of Blocking (Postcoat) Solution to each well.
 - B. Incubate 60 minutes.
 - C. After incubation, remove the Blocking (Postcoat) Solution and wash each well three times as in Step B1.5.
3. Standards and Samples
 - A. Dilute the standards in Sample Diluent according to the chart below:

Step	Ng/ml	Calibrator	Sample Diluent
0	50,000	5 µl	495 ul
1	250	5 µl from step 0	995 ul
2	125	500 ul from step 1	500 ul
3	62.5	500 ul from step 2	500 ul
4	31.25	500 ul from step 3	500 ul
5	15.6	500 ul from step 4	500 ul
6	7.8	500 ul from step 5	500 ul
7	3.9	500 ul from step 6	500 ul


- B. Dilute the samples, based on the expected concentration of the analyte, to fall within the concentration range of the standards.

- C. Transfer 100 µl of standard or sample to assigned wells.
 - D. Incubate plate 60 minutes.
 - E. After incubation, remove samples and standards and wash each well 5 times as in Step B1.5.
- 4. HRP Detection Antibody**
- A. Dilute the HRP conjugate in Conjugate Diluent. Recommended starting dilution is 1:10,000. Adjustments in dilution may be needed depending on substrate used, incubation time, and age of kit.
 - B. Transfer 100 µl to each well.
 - C. Incubate 60 minutes.
 - D. After incubation, remove HRP Conjugate and wash each well 5 times as in Step B1.5.
- 5. Enzyme Substrate Reaction**
- A. Prepare the substrate solution according to the manufacturer's recommendation.
 - B. Transfer 100 µl of substrate solution to each well.
 - C. Incubate plate 5-30 minutes.
 - D. To stop the TMB reaction, apply 100 µl of 2 M H₂SO₄ to each well. If using another substrate, use the stop solution recommended by manufacturer.
- 6. Plate Reading**
- Using a microtiter plate reader, read the plate at the wavelength that is appropriate for the substrate used (450 nm for TMB).

Calculation of Results

1. Average the duplicate readings from each standard, control, and sample.
2. Subtract the zero reading from each averaged value above.
3. Create a standard curve by reducing the data using computer software capable of generating a four parameter logistic (4-PL) curve-fit. Other curve fits may also be used.
4. A standard curve should be generated for each set of samples. See example below:

Orosomuroid (Alpha 1 Acid Glycoprotein) Standard Curve

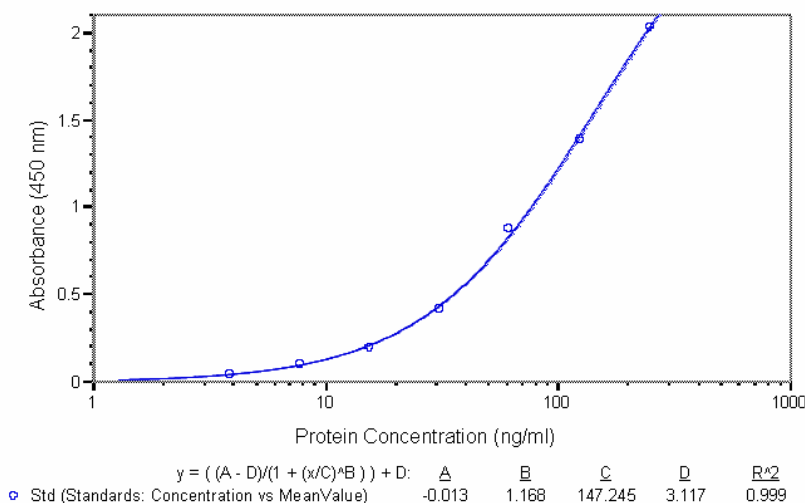

Orosomuroid Standards (ng/ml)

Sample	Concentration	BackCalcConc	Wells	Values	MeanValue	Std.Dev.	CV%
St01	250	248.253 255.54	A9 A10	2.015 2.039	2.027	0.017	0.8
St02	125	122.433 120.949	B9 B10	1.384 1.373	1.379	0.008	0.6
St03	62.5	63.954 68.062	C9 C10	0.845 0.891	0.868	0.033	3.7
St04	31.25	29.329 29.891	D9 D10	0.4 0.408	0.404	0.006	1.4
St05	15.625	14.561 15.373	E9 E10	0.184 0.196	0.19	0.008	4.5
St06	7.813	7.769 8.61	F9 F10	0.085 0.097	0.091	0.008	9.3
St07	3.906	4.443 4.292	G9 G10	0.039 0.037	0.038	0.001	3.7

Smallest Standard Value: 0.038

Largest Standard Value: 2.027

Technical Hints

1. The Capture antibody should be diluted with coating buffer immediately prior to its addition to the wells. Coated plates are stable overnight at 4°C when covered.
2. Change pipette tips between each addition of standard, sample and reagents to avoid cross-contamination.
3. Standards and samples should be pipetted to the bottom of the wells and all other reagents should be added to the side of the wells to avoid contamination.
4. Ensure that all buffers are not contaminated or expired. When troubleshooting ELISA results, it is recommended to prepare all new buffers in new vessels.
5. Do not add Sodium Azide to any of the buffers.
6. Sample and Conjugate dilutions should be made shortly before use.
7. Wash buffer should be aspirated from wells, as pouring wash buffer from wells may cause cross-contamination.
8. When preparing dilutions, wipe excess antibody/analyte from pipette tips to ensure accurate dilutions.
9. Incubation time of the Enzyme Substrate will depend on the substrate used and the intensity of the color change. The high standard should have an O.D. reading of about 2.0 and the low standard should have an O.D. reading above background.
10. The Stopping solution should be added to the wells in the same order as the Enzyme Substrate.

Troubleshooting

The following are some common problems encountered with the use of ELISA kits, and some of the causes of these problems.

1. **Problem: Low absorbance**
 - Incorrect dilutions or pipetting errors.
 - Improper incubation times
 - Improper mixing of the TMB substrate. Each component is mixed in equal parts.
 - Wrong filter on microtiter reader. Wavelength should be 450 nm for TMB, 490 nm for OPD, or 405 nm for ABTS.
 - Kit materials or reagents are contaminated or expired.

- Incorrect reagents used.

2. Problem: High Absorbance

- Cross contamination from other samples or positive control.
- Incorrect dilutions or pipetting errors.
- Improper washing.
- Wrong filter on microtiter reader.
- Contaminated buffers or enzyme substrate.
- Improper incubation times.
- Kit materials or reagents are contaminated or expired.

3. Problem: Poor Duplicates

- Poor mixing of specimens.
- Incorrect dilutions or pipetting errors.
- Technical error.
- Inconsistency in following ELISA protocol.
- Inefficient washing.

4. Problem: All wells are positive

- Contaminated buffers or enzyme substrate.
- Incorrect dilutions or pipetting errors.
- Kit materials or reagents are contaminated or expired.
- Inefficient washing.

5. Problem: All wells are negative

- Procedure not followed correctly.
- Contaminated buffers or enzyme substrate.
- Contaminated conjugate.
- Kit materials or reagents are contaminated or expired.